

TECHNICAL DATAS OF SYRINGE 50/60ML FOR SINGLE USE

MANUFACTURER: I.M.I. SNC DI MAZZUCATO PAOLO, ENRICO & C. – VIALE DELL'ARTIGIANATO VICOLO I° - 35036 MONTEGROTTO TERME (PD) – ITALIA

N° IDENTIFICATION CE: 0373 NUMBER OF THE CERTIFICATE: QPZ-1931-20 CLASS: Ila CND / EMDN CLASSIFICATION: A020102020101 N° REGISTRATION REPERTORY D.M.: 59510 (Italian registration) **REF. PRODUCT: ML99NA** LABEL: IMI VOLUME: 50/60ML NOZZLE: LUER LOCK MOUNTED NEEDLE: 14G BARREL: ATOXIC POLYPROPYLENE ADDED OF MASTER BATCH ORANGE COLOR PLUNGER: POLYPROPYLENE ATOXIC ADDED OF MASTER BATCH WHITE COLOR SEAL GASKET DOUBLE RING: MADE OF SYNTHETIC POLYSOPRENE BLACK COLOR SCALE: MARKED EACH ML IN BLUE COLOR FOR DRYING PROCESS BY UV LED SILICONIC OIL: MEDICAL FLUID PRIMARY PACKAGE: BLISTER OF MEDICAL PAPER AND COUPLED FILM SECONDARY PACKAGE: BOX OF TRIPLE CARTON RECYCLABLE x 50 PCS cm 38.0x24.5x19.5 OUTSIDE CARTON: TRIPLE CARTON RECYCLABLE x 300 PCS cm 60.0x39.0x49.5 STERILIZATION: BY ETHYLENE OXYDE SHELF LIFE: 5 YEARS DELIVERY: ON PALLETT 120x80x210 INCLUDING 16 OUTSIDE CARTONS MANUFACTURE: ACCORDING TO A QUALITY SYSTEM THAT ACCOMPLISHES ANNEX V° OF DIRECTIVE 93/42/CEE

NOTE: SYRINGES ARE PVC FREE, LATEX FREE. ALL USED SUBSTANCES ACCOMPLISH WITH REGULATION EC 1907/2006 REACH.

INSTRUCTION FOR USE:

- 1. Sterile only in undamaged package.
- 2. Use the syringe immediately after the aspiration of the fluid.
- 3. Move the plunger only in sterile place.
- 4. Single use.
- 5. Do not sterilize again.
- 6. Throw away syringe after use.


STABILITY:

Stock of products: keep the material in cool and dry place (temperature +5 ...+35°C – H.R. 30/70%) For the protection from bright sources is sufficient to keep the product in its blister.

INTENDED USE:

Injection therapy and infusional therapy (on driven syringes' pump) with light sensitive liquids

ACCORDING TO THE FOLLOWING STANDARDS: ISO 594-1 ISO 594-2 ISO 7886-1 ISO 7886-2 (COMPATIBLE WITH PUMP'S SETTING B.BRAUN OMNIFIX) ISO 10993 UNI EN ISO 11135 UNI EN ISO 556 EUROPEAN PHARMACOPOEIAE EUROPEAN DIRECTIVE 93/42 CEE

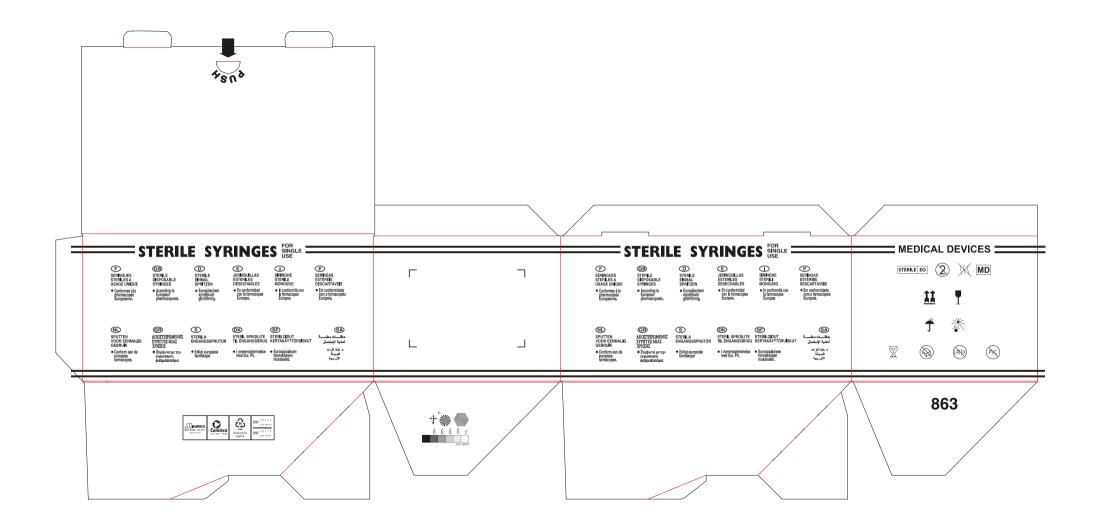

STERILE SYRINGES	MEDICAL DEVICES	STERILE SYRINGES	MEDICAL DEVICES
STERLIC MD P <	ETEREE X MO ®	TUTULE CO Image: Constraint of the second	 ★★ ★★
	0963		+,⊛ ■ <u>* * ((()</u>